



CONTENTS

WELCOME TO SOTA	3
BEFORE USING	3
LEARN MORE	3
COMPLETE UNIT INCLUDES.....	3
DO NOT USE.....	4
MICROPULSING CAUTIONS	4
IONIC~COLLOIDAL SILVER CAUTIONS.....	5
GENERAL CAUTION.....	5
SUMMARY OF LIGHTS	5
HOW TO USE THE MICROPULSING FUNCTION	6
How Micropulsing Should Feel	9
Sensitive Skin	10
Typical Use	10
HOW TO USE THE IONIC~COLLOIDAL SILVER FUNCTION	11
How to Assemble	11
How to Make Ionic~Colloidal Silver.....	11
Typical Use.....	13
ELECTRICAL SPECIFICATIONS	13
Power Requirements.....	13



Optional Power Input..... 13

Output Specifications..... 14

TROUBLESHOOTING..... 14

COUNTRIES THAT PARTICIPATE IN MANUFACTURING..... 14

REPLACEMENT ACCESSORIES..... 14

WARRANTY..... 14

REPAIRS..... 15

WELCOME TO SOTA

Thank you for allowing us to be a part of your Wellness Team.

The Silver Pulser is a consumer product designed to be used as part of a Wellness Lifestyle. A commitment to healthy lifestyle choices is an important factor in the journey to Wellness.

The SOTA Silver Pulser has two functions – Micropulsing and making Ionic~Colloidal Silver. Micropulsing offers gentle microcurrents that work with the body's natural electricity for more energy, general health and well-being. Ionic~Colloidal Silver is one of nature's gifts and can be made easily and inexpensively at home.

The Silver Pulser is designed to be used independently, but can also be used together with any of the SOTA Products.

With proper care, your Silver Pulser should provide you many years of trouble-free use.

Please understand that results will vary.

BEFORE USING

Please read this manual thoroughly before using your Silver Pulser. For the most up-to-date manual, please visit our website www.sota.com/manuals.

We've made every effort to ensure the information in your manual is up-to-date at the time of printing ... since that time however, new information may have become available.

LEARN MORE


To learn more about the Silver Pulser we invite you to visit the SOTA website:

www.sota.com

The website offers How to Videos, Frequently Asked Questions, *The SOTA Products User Guide*, SOTA News ... and more.

COMPLETE UNIT INCLUDES

- One (1) Silver Pulser Unit
- One (1) 9-Volt Alkaline Battery

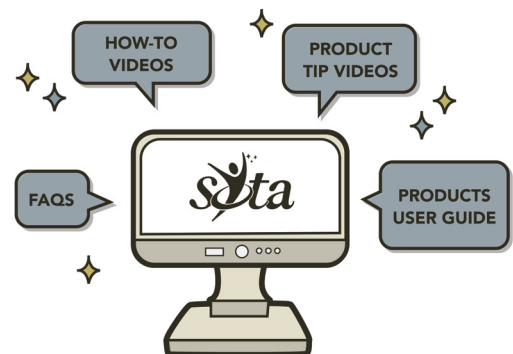

- One (1) Carrying Case
- One (1) Product Manual

FOR MICROPULSING APPLICATION:

- One (1) Micropulsing Cord for Rubber Probes
- Two (2) Pair Conductive Rubber Probes
- Six (6) Pair Cotton Sleeves with Velcro®
- One (1) Arm Band and Clip
- One (1) Neoprene® Velcro® Wrist Strap
- One (1) 50 ml Dark Glass Dropper Bottle

FOR MAKING IONIC~COLLOIDAL SILVER:

- One (1) Silver Wire Holder
- Two (2) Silver Wires of .9999 (4 Nine) Purity
- One (1) Green Scrub Pad

DO NOT USE

1. Do not use in the following situations as safety has not been explored using the Micropulsing function:
 - a. In the case of pregnancy.
 - b. With an active implanted device such as a pacemaker, etc.
2. As with all electrical products do not use near water, when driving a car or when operating heavy equipment.
3. Do not connect the Micropulsing Cord or the Silver Wire Holder to any other USB outlet, such as a computer or power supply. Do not plug any other USB connections into the Silver Pulser, other than the Micropulsing Cord and the Silver Wire Holder.

MICROPULSING CAUTIONS

1. Do not place the Conductive Rubber Probes over skin lesions, abrasions, new scars, cuts, eruptions or sunburn.
2. Discontinue use if the Micropulsing suddenly feels different or prickly **and** the YELLOW light stops flashing. Turn the unit OFF and contact SOTA.

3. Caution is advised if using potentially harmful substances such as recreational and prescription drugs, as it is not known if microcurrents will interact or if individual reactions may occur.
4. Caution is required in the following situations as a burn may occur, which could scar:
 - a. Do not apply the bare metal pins to the skin.
 - b. Allowing the Cotton Sleeves to dry out while Micropulsing.
 - c. Sleeping while Micropulsing, as the Cotton Sleeves may dry out.

IONIC~COLLOIDAL SILVER CAUTIONS

We recommend taking occasional breaks from consuming Ionic~Colloidal Silver for the following reason:

A handful of people have experienced argyria after drinking large amounts of Ionic~Colloidal Silver daily, over a long period of time. Argyria is a bluish tinge of the skin. This occurs when excess silver is eliminated through the skin and exposed to light. Darkening of the moons of the finger nails is usually an early sign.

The risk of argyria is considered greater for those who are ingesting incorrectly made Ionic~Colloidal Silver and to a lesser degree, those who are deficient in selenium or vitamin E.

When making and drinking Ionic~Colloidal Silver as currently recommended by SOTA, the risk of argyria is extremely rare. Please see www.sota.com/manuals.

GENERAL CAUTION

While this technology is generally considered safe, there exists potential for rare individual reactions that cannot reasonably be foreseen. Therefore, your use of the SOTA Products constitutes your agreement that you are responsible for your decision to use the technology. SOTA assumes no responsibility for any direct or indirect loss or damage believed to arise from using the SOTA Products.

SUMMARY OF LIGHTS

GREEN: Indicates the unit is on.

RED: Indicates the battery is low and will soon need replacing.

YELLOW: Indicates the Micropulsing function is in operation.

ORANGE: Indicates the Ionic~Colloidal Silver function is in operation.



HOW TO USE THE MICROPULSING FUNCTION

1. Place the 9-Volt Alkaline battery in the unit.
 - a. On the back of the unit, slide off the battery cover.

- b. Position the 9-Volt Alkaline battery so the positive (+) and negative (-) terminals line up as in image 1.

Note: The smaller circle on the battery matches the smaller circle in the case ... the larger battery circle matches the larger circle in the case.

- c. Slide the 9-Volt Alkaline battery into the case and push down. Slide the cover back onto the unit.

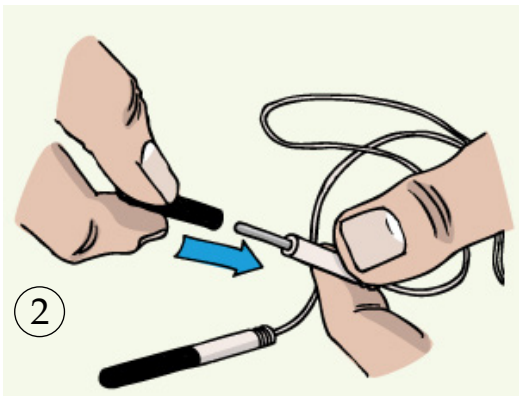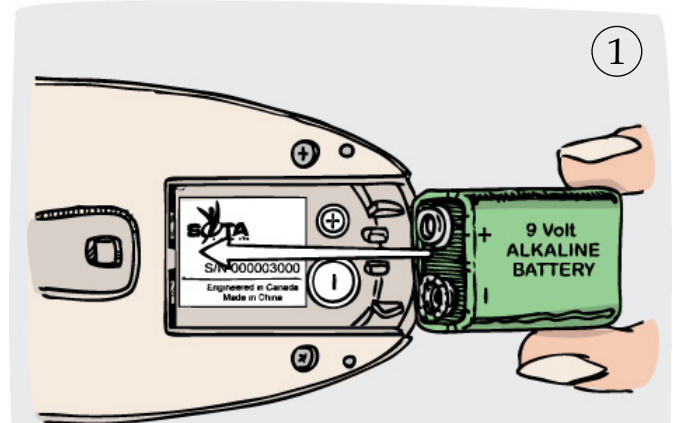


2. Attach the Conductive Rubber Probes to the Micropulsing Cord by gently sliding the Rubber Probes over the metal pins on the Micropulsing Cord, as in image 2.

Note: Except to occasionally clean them, the Rubber Probes can stay on the Micropulsing Cord between uses.

3. Clean the wrist area to remove oils from the skin. This will allow for better conductivity.
4. Insert the Micropulsing Cord into the jack on the unit as shown in image 3. The USB symbol on the plug should be facing up. When the plug is positioned correctly, it will slide in gently. Do not force.


5. Slide the clip on the back of the Silver Pulser into the holding clip on the Arm Band as in image 4 on page 7.

6. Slide the Arm Band, with the unit and cord, up the arm to a comfortable position. Tighten the band to secure it in place as in image 5 on page 7.

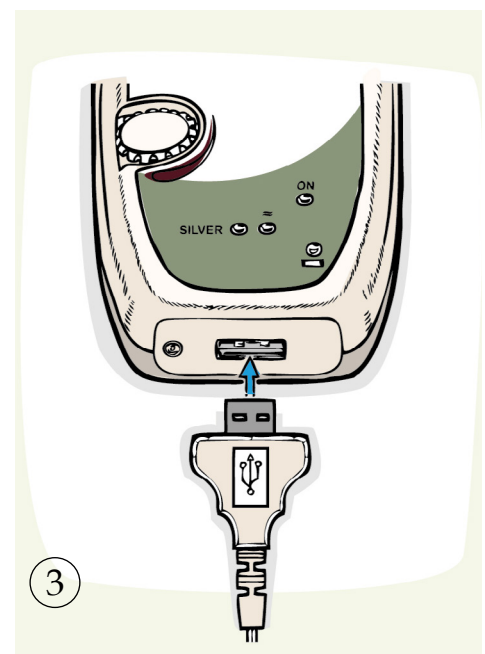


Option: If preferred the unit can be placed in a pocket. A longer Micropulsing Cord is needed for this option.

7. Put the Wrist Strap on with the Velcro® side of the Wrist Strap face-out rather than towards the skin.
8. Prepare one pair of Cotton Sleeves. Each Cotton Sleeve is sewn on three sides; to find the open end of the Cotton Sleeve, squeeze the long sides of the sleeve and the unsewn end will pop open.
9. Attach one Cotton Sleeve to the Wrist Strap in line with the pulse point on the thumb side of the wrist. The open end of the Cotton Sleeve will point down toward the elbow. Press the sleeve to the Wrist Strap to firmly adhere the sleeve in place.

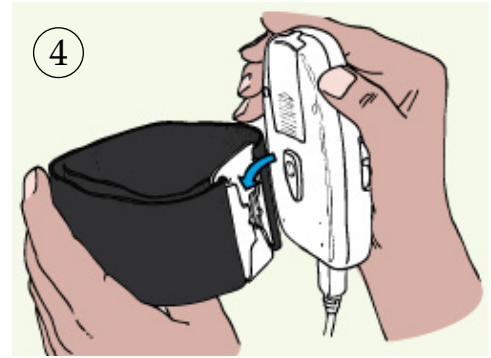

10. Place the other Cotton Sleeve, again with the open side towards the elbow, in line with the pulse point on the little finger side of the wrist. This pulse point is usually harder to feel. It is located in the soft hollow on the wrist, in line with the little finger. Press the sleeve to the Wrist Strap to firmly adhere the sleeve in place. See image 6.

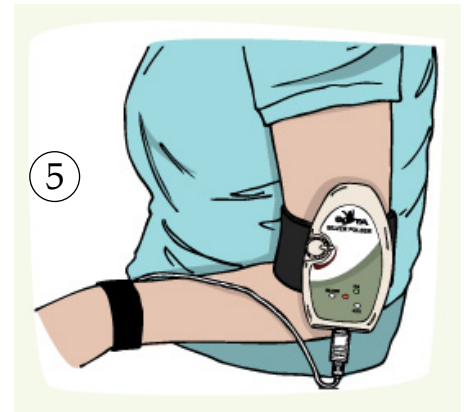


11. Take the Wrist Strap off.
12. Insert one probe from the Micropulsing Cord into the open end of each Cotton Sleeve. Use a gentle twisting motion to work the Rubber Probes into the Cotton Sleeves.


13. Wet the Cotton Sleeves with water.

14. Put the Wrist Strap on so the damp Cotton Sleeves are against the skin over the pulse points. See image 7 on page 8.

15. Turn the unit ON by rotating the ON/OFF switch clockwise. Turn the switch slowly until you feel the current. If you do not feel the current, see 'Notes' on page 8.

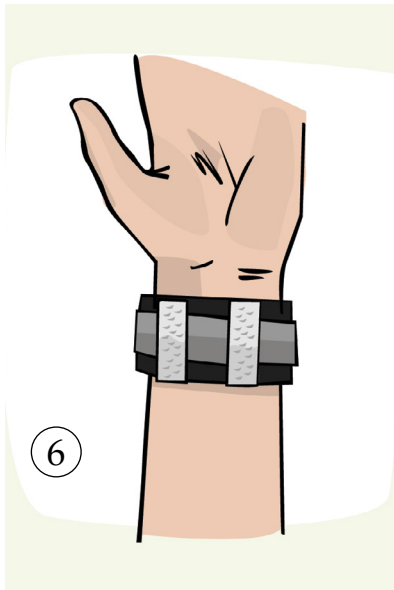


- a. The GREEN light indicates the unit is ON. If the light does not come on, the battery may not be placed correctly.
 - b. The flashing YELLOW light should come on and get brighter as the intensity is turned up. If the flashing YELLOW light does not come on, the electrical path has not been established. See 'Troubleshooting' on page 14.
16. When finished, turn the unit OFF by rotating the ON/OFF switch counter clockwise until it clicks. Do not force the ON/OFF switch past its natural stopping point.
17. Unplug the Micropulsing Cord. Do not store the unit with the Micropulsing Cord plugged in as this can damage the Cord.
18. The Cotton Sleeves will remain correctly positioned for the next session.
19. Clean the wrist and apply a healing lotion to avoid irritation.

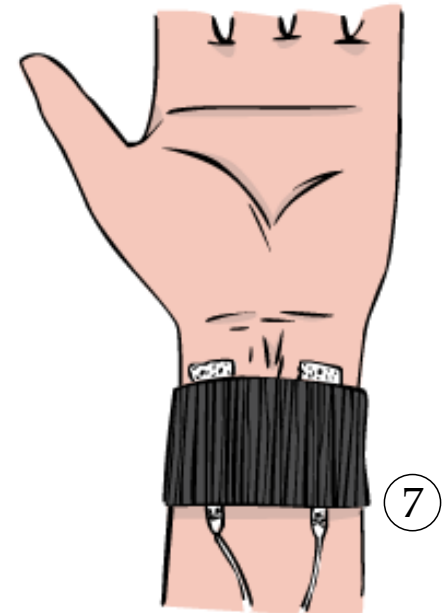

Notes:

Suggestions for Feeling the Current: If the current is not felt with wet Cotton Sleeves, prepare a mild salt solution to wet the sleeves. Add a few grains of salt to the water in the 50 ml dropper bottle. Alternatively, a conductive gel or aloe vera gel may be used instead of a salt solution. Drink enough water to keep the body well hydrated. The level of hydration may affect sensitivity.

Care of Micropulsing Cord and Rubber Probes: Remove the Rubber Probes occasionally to clean in a mild soap solution. Rinse thoroughly. If necessary, gently wipe the metal pins of the Micropulsing Cord.

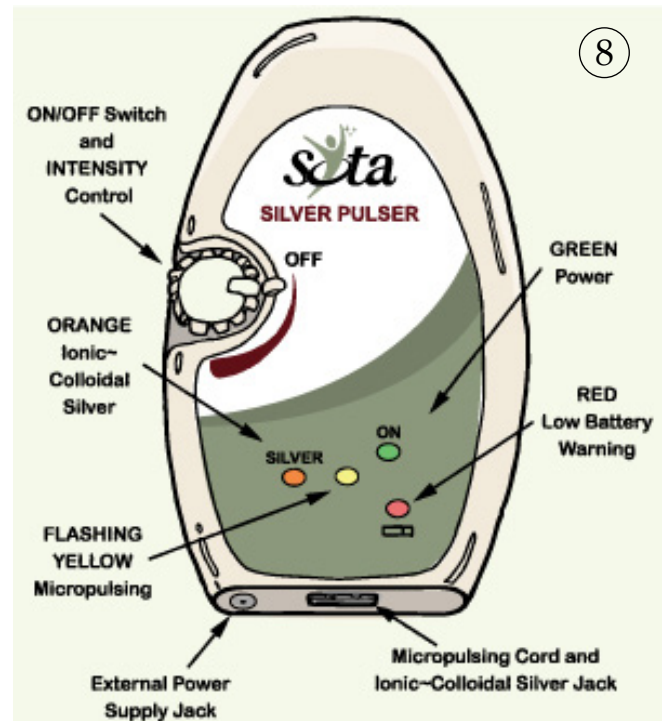

Care of Cotton Sleeves: Wash or rinse sleeves occasionally. Discard and replace Cotton Sleeves periodically.

Alternatives to Cotton Sleeves: The following items can be used in place of the Cotton Sleeves with Velcro®:

- a. All Cotton Sleeves: SOTA also offers Cotton Sleeves without Velcro®.
- b. Unbleached Paper Towel: Cut a small square of paper towel large enough to wrap around the Rubber Probe 2 or 3 times. Moisten prior to use.
- c. Cotton Flannel: Cut a small square of cotton flannel and wrap around the Rubber Probe with thread. Moisten prior to use.

Rubber Probes: Over time, the Rubber Probes will lose their conductivity and need replacing. Refer to the SP7 Troubleshooting Guide for instructions on how to test the Rubber Probes.

Low Battery Warning: The RED light comes on and the unit will beep when the battery is low. This means the battery will soon need to be replaced. The battery can continue to be used until the YELLOW light goes off.

Power Supply: When Micropulsing, as a safety feature, the unit can only be powered by a 9-Volt battery.

Replacement Batteries: When purchasing replacement 9-Volt batteries, take the Silver Pulser with you to ensure a proper fit, as 9-Volt batteries vary in size.

HOW MICROPULSING SHOULD FEEL

1. The sensation is a gentle pulsing. While the microcurrents should be felt, it is not necessary to turn the intensity control up to an uncomfortable level.
2. With repeated use, the ability to feel the microcurrents may change. It may be necessary to increase the intensity in order to feel the microcurrents.
3. Twitching of the fingers is normal at a higher intensity.
4. During the first weeks of use, the skin may become irritated. Over time, irritation usually decreases or disappears. Alternating wrists each session allows any irritation to better heal.

SENSITIVE SKIN

Some individuals may be particularly sensitive to microcurrents and the irritation may continue. To minimize irritation:

1. Wash wrists thoroughly after each session and apply a healing gel or lotion such as aloe vera, vitamin E or MSM cream.
2. Micropulse for shorter periods of time until the irritation disappears.
3. Alternate wrists daily.
4. Wet the Cotton Sleeves with distilled water or Ionic~Colloidal Silver. If unable to feel the current, try a commercial saline solution for the eyes. This is gentler than adding salt to the water.
5. A conductive gel or aloe vera gel added to the wet sleeves may help to reduce irritation.
6. Another option is to wrap a small square of paper towel around the Rubber Probes instead of using Cotton Sleeves. Keep the paper well moistened. A small square of paper towel may last for several applications. If available, use unbleached paper towel.
7. Set the intensity dial to a comfortable level. The YELLOW flashing light needs to be visible indicating the current is flowing.

TYPICAL USE

Alternate wrists daily.

Length of Session: Build up time gradually. It is best to start slowly. Start with 10 to 20 minutes a day. Increase gradually to a minimum of 2 hours each day.

Length of Use: Use daily for a minimum of 8 to 12 weeks. Once completed, setting a schedule for ongoing use is beneficial. Suggestions for a maintenance schedule are a) 1 to 3 times per week, b) 1 week per month, or as needed. The initial program can be repeated at any time.


Drink Plenty of Water: It's important to drink enough water when using the unit. Drinking ozonated water is especially helpful.

Stop Gradually: Reduce the amount of time each day for the last week of use. If using the 4-part SOTA Protocol, it is suggested to stop only one part of the protocol at a time.

HOW TO USE THE IONIC~COLLOIDAL SILVER FUNCTION

HOW TO ASSEMBLE


1. The Silver Wires fit into the two small holes in the Silver Wire Holder.
2. To insert the Silver Wires, move the spring clip away from the hole to allow the wire to slide in smoothly.
 - a. Insert as in the picture. Push the wire through. Most of the wire should be below the holder. It may be easier to insert from the underside of the holder.
 - b. Release the clip to hold the Silver Wire snugly in place.
3. Repeat the above steps for the second Silver Wire and plug the Silver Wire Holder into the Silver Pulser, ensuring that the USB symbol on the plug is facing up.

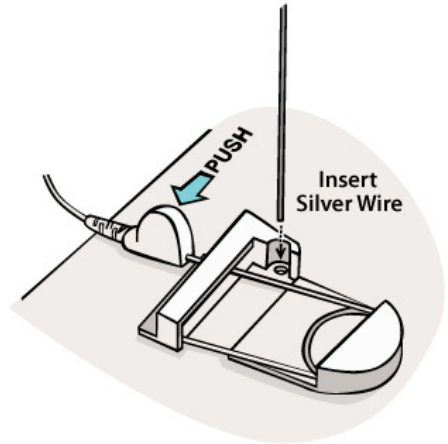

HOW TO MAKE IONIC~COLLOIDAL SILVER

The Silver Pulser provides a constant current output, which allows for a very simple procedure for making a high quality Ionic~Colloidal Silver using room temperature water.

1. Pour two cups (16 ounces or 500 ml) of room temperature distilled water into a tall glass container. Do not use a metal or plastic container.
2. Place the Silver Wire Holder on the glass container immersing at least 70% of the Silver Wires into the water. Keep them at least 25 mm or 1 inch from the bottom of the container.
3. Turn the unit ON by rotating the ON/OFF switch clockwise until it clicks. It is not necessary to turn up the intensity.

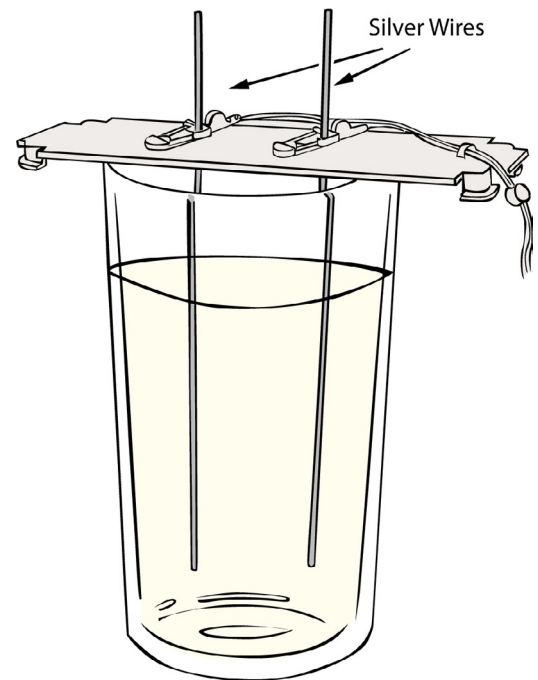

The ORANGE light will brighten as the current increases up to the 1.0 mA limit.

4. Stir occasionally with a non-metal utensil. Occasionally, wipe off the grey or black

silver oxide that builds up on the Silver Wires.

- Two cups (16 ounces or 500 ml) for 2 hours will produce a 5 to 8 ppm batch of Ionic~Colloidal Silver, depending on the brand of distilled water. The concentration of silver is measured in parts per million or ppm.

Note: With constant current the time required to produce 5 ppm or more will not be reduced by adding salt or by heating the water. The current is held steady and is not influenced by salt or heat.

- When finished, wipe the Silver Wires with paper towel to remove residue. Buff lightly when needed to keep them free of sediment. Harsher buffing will wear away the silver faster.

Notes:

Color: Ionic~Colloidal Silver remains colorless to about 5 or 6 ppm. At a slightly higher ppm it will be a pale gold color. Do not drink if it is darker than pale gold or dark grey as this indicates a higher level of impurities or larger particle sizes.

Clarity: The electrolyte should be clear. Do not drink if it is cloudy.

To Make Larger Quantities: The Silver Pulser can be used to make larger quantities of Ionic~Colloidal Silver. For a concentration between 5 to 8 ppm, use the following times as a guide:

For 4 cups or 1 liter: 3 to 4 hours.

For 1 gallon (16 cups) or 4 liters: 10 to 12 hours.

Storage: Pour the Ionic~Colloidal Silver into a dark glass bottle – never metal – and store in a dark, dry place. Over time, light will degrade Ionic~Colloidal Silver by turning the electrolyte grey or black.

When made and stored properly, Ionic~Colloidal Silver retains freshness for many months. It is suggested, however, that you use as soon as possible. If settling occurs, it is losing potency. Do not drink any sediment.

Do not freeze, refrigerate, or expose Ionic~Colloidal Silver to extremes of temperatures as its potency may be affected.

Save on Batteries: The unit can be powered by an AC-DC wall adaptor when making Ionic~Colloidal Silver. See 'Optional Power Input' on page 13.

Switch Silver Wire Positions: The silver ions only come off the wire in the positive

(+) or anode terminal into the water. To equalize the wearing of the Silver Wires, exchange the position of the wires after each use. If left in the same position, only one Silver Wire will gradually wear away.

Replacing the Silver Wires: The Silver Wires are of the highest grade .9999 or 99.99% or 4 Nine pure fine silver. When the SOTA pure Silver Wires wear too thin, do not replace with sterling silver, as it contains nickel, which can be toxic.

TYPICAL USE

Quantity: There is no definite amount to drink. When consumed on a regular basis – daily or several times a week – it is best to drink no more than 1 to 2 ounces (30 to 60 ml) at a time.

Larger amounts of Ionic~Colloidal Silver – 1 cup or more – can be consumed for short periods of time, for example, a few weeks. It is better to take smaller amounts throughout the day rather than all at once.

Length of Use: 1 to 2 ounces (30 to 60 ml) or more daily for 2 or 3 months. Ionic~Colloidal Silver can be used as needed. The initial program can be repeated at any time. If using for an extended period, it is wise to take breaks.

Strength: Laboratory testing indicates Ionic~Colloidal Silver is effective as low as 2 ppm. When ingesting on a regular basis, it is suggested to limit the strength to less than 10 ppm.

ELECTRICAL SPECIFICATIONS

POWER REQUIREMENTS

Use a 9-Volt Alkaline battery for proper operation.

OPTIONAL POWER INPUT

Both functions of the Silver Pulser can also be operated using rechargeable batteries. When purchasing rechargeable batteries, it is suggested to take the unit with you to ensure the batteries will fit the enclosure.

To use a wall adaptor for making Ionic~Colloidal Silver the output should be from 6 to 12 Volts DC with a **Tip or Center Positive** pin and a minimum of 500 mA (milliamperes) of current. The wall adaptor that comes with other SOTA units can be used for making Ionic~Colloidal Silver.

Caution: Exceeding the voltage rating or reverse connection may result in injury or unit failure. This will **void** the warranty.

To operate the Ionic~Colloidal Silver Function from a 12 Volt DC source, such as an automobile battery or an appropriate Solar Panel, purchase a Universal Power Cord with **Tip or Center Positive**.

OUTPUT SPECIFICATIONS

The output voltage is a nominal 31 Volts.

Micropulsing Application: Frequency through the metal pins is ~3.92 Hz or $\frac{1}{2}$ of the Earth Schumann frequency of 7.83 Hz, (+/- 1 Hz) with a Bi-Phasic Square Wave @ 31 Volts (+/- 1 Volt) peak per cycle.

Maximum current through the metal pins is ~8 milliamperes into 1,000 ohms, ~12 milliamperes into a short circuit at 31 Volts peak per cycle.

Ionic~Colloidal Silver Application: The maximum current through the Silver Wires is 1.0 milliamperes (+/- 0.5 mA) at 31 VDC compliance voltage when the Silver Wires are touched together to short the circuit.

TROUBLESHOOTING

Troubleshooting Guides for both the Micropulsing and Ionic~Colloidal Silver Functions of the Silver Pulser are available at www.sota.com/manuals. These Guides are a great tool to check if you are experiencing any issues with your unit.

COUNTRIES THAT PARTICIPATE IN MANUFACTURING

The manufacturing of the SOTA Products is a global collaboration. The following countries have participated in the making of the Silver Pulser (listed in alphabetical order): **Canada, China, Hong Kong, Malaysia, Mexico, Taiwan, Thailand** and the **USA**

REPLACEMENT ACCESSORIES

To replace your accessories, please contact your supplier.

WARRANTY

The Silver Pulser Model SP7 is covered by a three (3) year limited warranty. Please keep proof of purchase. Warranty is void if the failure is due to abuse or negligence. SOTA reserves the right to make changes to the Silver Pulser without obligation.



REPAIRS

Please contact your supplier for return instructions. For information about your closest repair depot, contact repairs@sota.com or call Toll-Free: 1.800.224.0242 (Canada & USA) or 1.250.770.2023.



Made in China. Designed and Engineered in Canada.

• The SOTA units are consumer products designed to be used as part of a Wellness Lifestyle • The SOTA units are not medical devices nor are they intended to diagnose, treat or cure any medical or health condition • The use, safety or effectiveness of the SOTA units has not been approved by any government agency • Please consult a health practitioner for any medical or health condition • Results using the SOTA Products will vary for each person • Please note that all purchases of SOTA Products are deemed to be made in Penticton, BC, Canada •